

More than Just a Phase: Understanding Phase Stability in RF Test Cables

AN-46-004

I. Introduction

One important factor in ensuring accurate, repeatable measurements in RF test applications is the stability of performance of the test cable used. In most test environments, cables undergo frequent bending during normal use, which can result in changes in phase and other performance parameters. Depending on the cable, these changes can be significant enough to degrade the accuracy and precision of your measurements. Therefore, in choosing the right test cable for your needs, it's important to consider how bending affects cable phase performance and how a cable is (or isn't) qualified for stability of phase versus flexure.

This article will review the basics of phase stability in [RF coaxial cables](#) and identify the factors that affect phase performance. Two methods of testing phase change versus flexure will be explored, and the preferred method used to qualify Mini-Circuits' T40- and T50-series phase-stable cables presented and explained in detail.

II. Why Phase Matters

Phase stability is desirable in test cables because it:

- Ensures good phase tracking with changing temperature, and lowers residual errors and uncertainties
- Improves antenna gain for better system performance and accuracy
- Provides better bit error rate (BER) which increases effective range
- Extends the length of time between calibrations and minimizes drift between calibrations

III. What Causes Phase Change?

In general, phase is affected by the physical length of the cable assembly, the cable bend radius, and the cable assembly technique. Recall that the electrical length of an RF line in degrees is defined by:

$$\text{Electrical Length [deg]} = 360^\circ * \frac{L}{\lambda}$$
$$\text{And } \lambda = \frac{c}{\sqrt{\epsilon_r} f}$$

Where f is frequency in Hz, L is physical length in meters, ϵ_r is the dielectric constant of the cable material, c is the speed of light in meters per second, and λ is the wavelength.

Cables are typically designed to operate over a wide frequency range and minimize attenuation (loss). The longer the electrical length, the greater the loss. Since electrical length (and loss) is directly proportional to the square root of ϵ_r , most RF cables are manufactured from materials with a low dielectric constant, usually PTFE (Teflon) and in some cases SiO₂. PTFE is more common because it's easy to bend without damaging, while SiO₂ is brittle and only suitable for semi-rigid cable assemblies. All Mini-Circuits' cables use PTFE, as a good degree of flexibility is needed in most applications.

One drawback of the flexible PTFE construction is, of course, the potential for phase changes (and other performance changes) due to bending. Bending the cable changes the physical length at the point of bend. It may also constrict and loosen the dielectric, shielding, and braiding around the center conductor, which can also affect the electrical length and result in phase changes.

Depending on the design and construction, some cables will exhibit greater sensitivity of phase with bending than others. Mini-Circuits' T40- and T50-series cables are specifically designed and tested for stability of phase versus flexure. What follows will explain the methodology Mini-Circuits uses to qualify phase stability in these models.



*Figure 1: Mini-Circuits
T50-3FT-VFVM+ phase-stable
test cable*

IV. How Phase Change is Measured

Measuring phase change versus flexure involves connecting the cable to a VNA and sweeping phase across frequency with some setup to bend the cable into specified radii to show corresponding changes in phase. There are, of course, many setups we could conceive to measure phase stability, and the reliability of this parameter depends on the robustness of the test method used. Mini-Circuits has explored multiple test methods to determine the most reliable procedure to characterize phase stability in our test cables.

Unexpected Result from the “Cross-Bow” Two-Port Method

The cross-bow-like fixture shown in Figure 2 below was built as one possible solution for measurement of cable performance vs. flexure. The apparatus has two adjustable arms to support the connector ends when connected to VNA ports 1 and 2. The cable is wrapped around a 4 inch mandrel which slides along the scaled bar, creating the specified bend radius. Figure 2 pictures the setup with measurements being made on Mini-Circuits model T50-3FT-KMKM+ at 10”, 3.25”, and 2.4” radii.

We would expect the relationship between bend radius and phase change to be linear. However, the data collected on the cable using this method exhibited a parabolic-shaped phase vs. flexure curve. This result is likely due to the multiple radial bends in the cable in this configuration: two in one direction, and one in the opposite direction. The data from this test is unusable because it gives the appearance of the cable being more resistant to phase change in tighter bends, which deviates from the expected performance.

Preferred Procedure: The One-Port Method for Testing

In the setup pictured in Figure 4, one-port calibration was performed on the VNA. The DUT (cable T50-3FT-KMKM+) was connected to the VNA and terminated at the end with a short. The VNA was then normalized in the straight position. The cable was then wrapped one full turn (360°) around a mandrel of specified radius in one direction, and measurement was taken by sweeping phase across frequency. The cable was straightened, and the VNA normalized again. A second measurement was taken with the cable wrapped one full turn in the opposite direction, around a second mandrel on the opposite side. This procedure was repeated for radii of 2” and 3”.

The data collected on the cable using this method exhibited the expected linear relationship between phase change and flexure (Figure 5). This method avoids any effects of additional bends in the cable and other factors that may distort the measurement, and the data is usable.

V. Conclusion

The measurement of phase versus flexure varies from company to company in the RF cable industry, and it's important to understand how manufacturers specify phase stability when selecting a cable for an application in which this is a desired feature. Mini-Circuits uses the one-port method explained above to test phase stability in all of our T40- and T50-series [phase-stable RF test cables](#). Data from this test is presented on the datasheet for all models in these families.

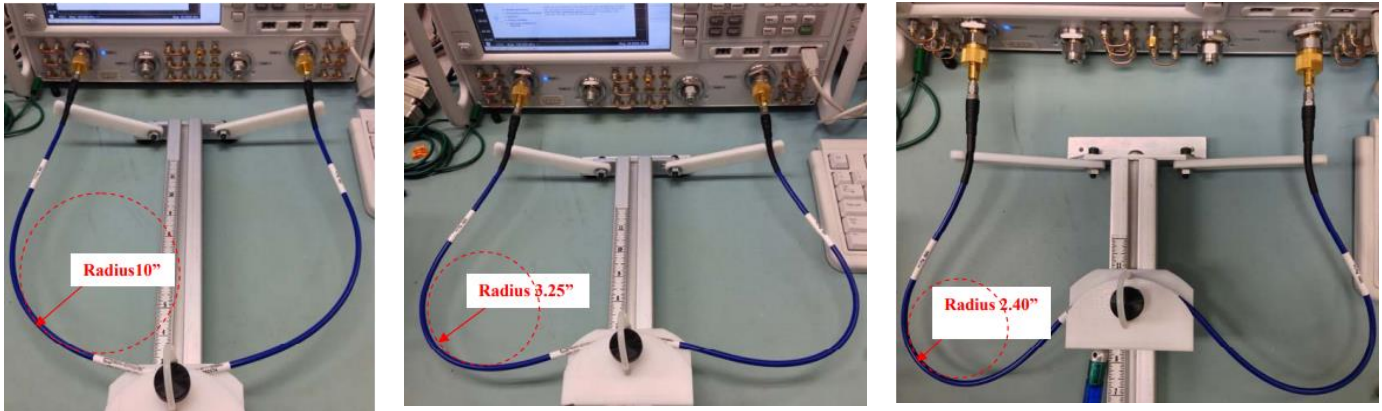


Figure 1: "Cross Bow" apparatus for measuring cable performance versus bend at 10", 3.25", and 2.4" bend radii.

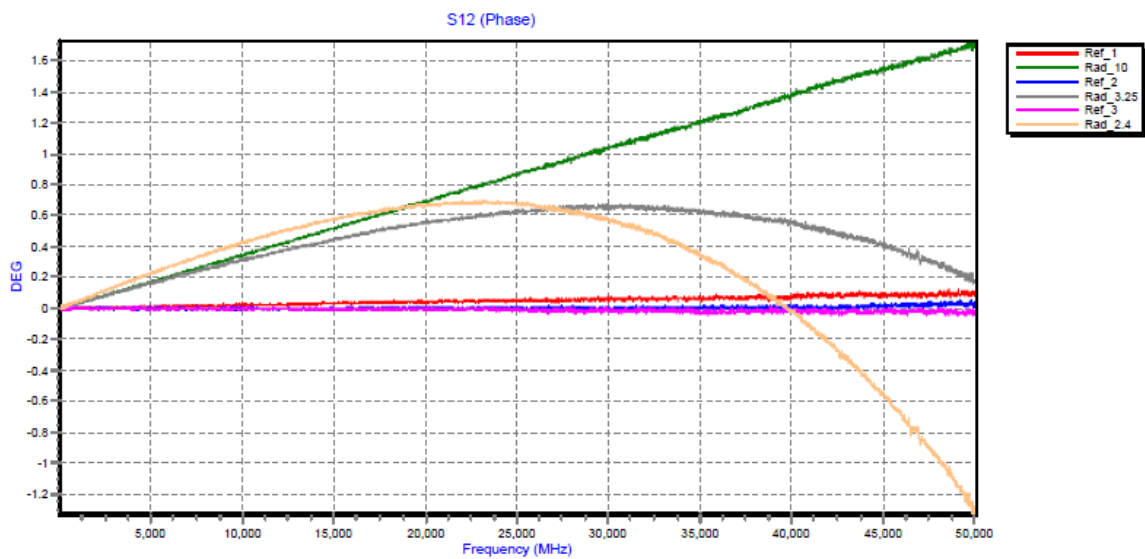


Figure 2: T50-3FT-KMKM+ using the "cross-bow" two port method, exhibiting a parabolic relationship between phase change and flexure.

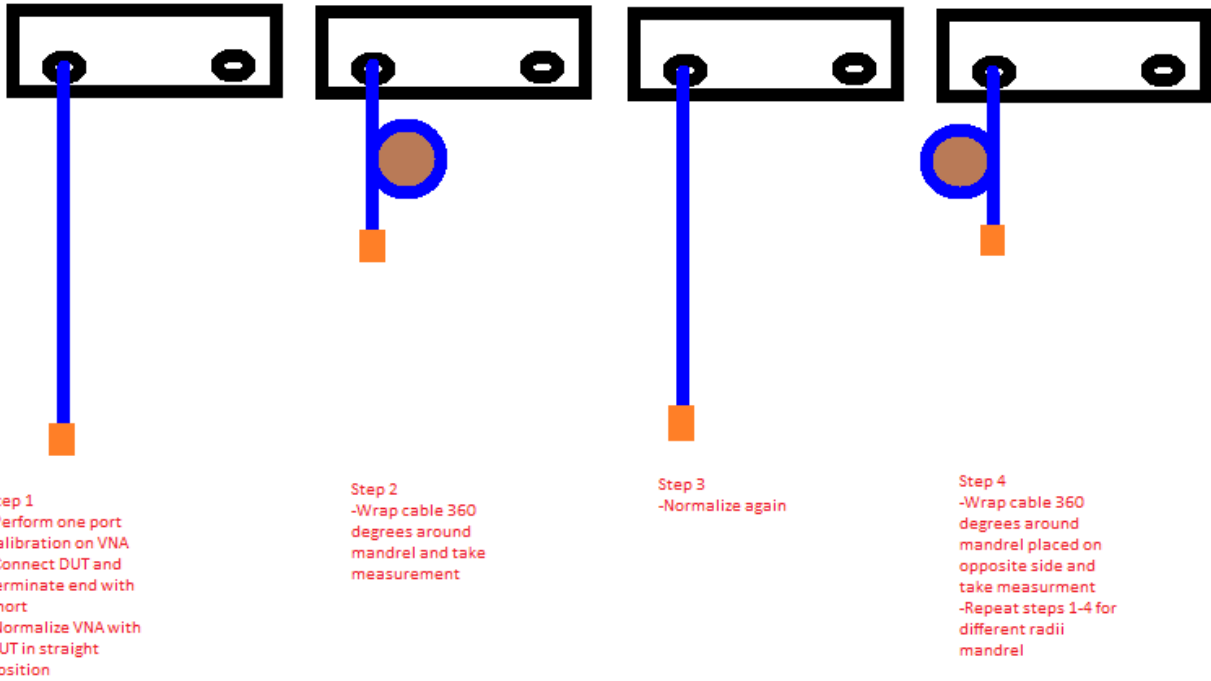


Figure 3: Simple visualization of the one-port method for testing phase stability vs. flexure.

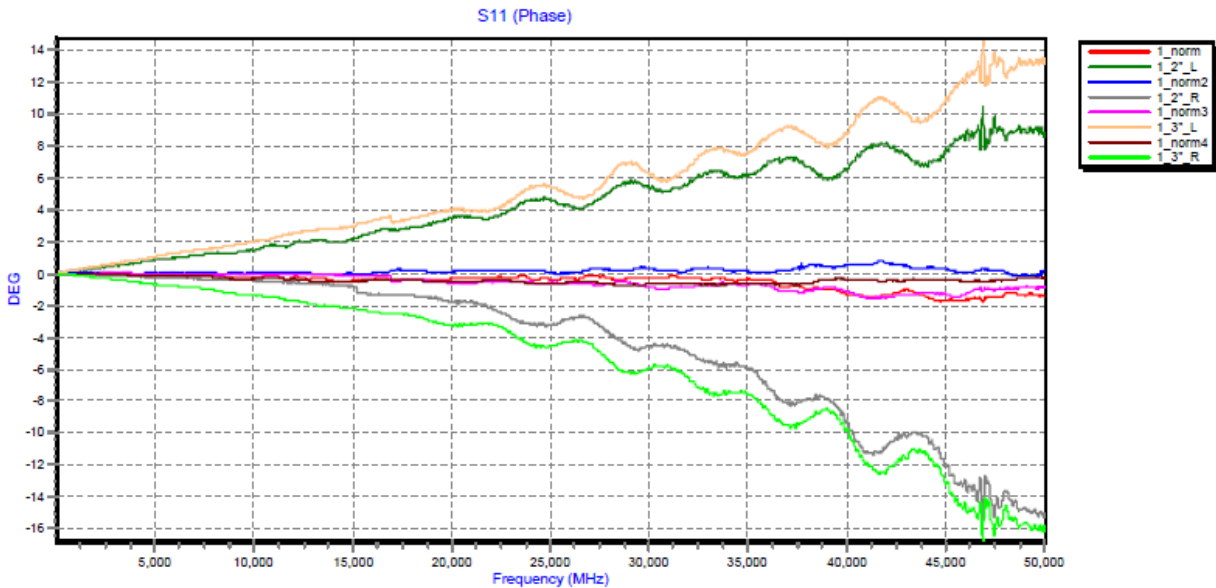


Figure 4: T50-3FT-KMKM+ using the one-port method, exhibiting the expected relationship between phase change and flexure. *S11 halved to obtain phase change.

IMPORTANT NOTICE

© 2017 Mini-Circuits

This document is provided as an accommodation to Mini-Circuits customers in connection with Mini-Circuits parts only. In that regard, this document is for informational and guideline purposes only. Mini-Circuits assumes no responsibility for errors or omissions in this document or for any information contained herein.

Mini-Circuits may change this document or the Mini-Circuits parts referenced herein (collectively, the "Materials") from time to time, without notice. Mini-Circuits makes no commitment to update or correct any of the Materials, and Mini-Circuits shall have no responsibility whatsoever on account of any updates or corrections to the Materials or Mini-Circuits' failure to do so.

Mini-Circuits customers are solely responsible for the products, systems, and applications in which Mini-Circuits parts are incorporated or used. In that regard, customers are responsible for consulting with their own engineers and other appropriate professionals who are familiar with the specific products and systems into which Mini-Circuits' parts are to be incorporated or used so that the proper selection, installation/integration, use and safeguards are made. Accordingly, Mini-Circuits assumes no liability therefore.

In addition, your use of this document and the information contained herein is subject to Mini-Circuits' standard terms of use, which are available at Mini-Circuits' website at www.minicircuits.com/homepage/terms_of_use.html.

Mini-Circuits and the Mini-Circuits logo are registered trademarks of Scientific Components Corporation d/b/a Mini-Circuits. All other third-party trademarks are the property of their respective owners. A reference to any third-party trademark does not constitute or imply any endorsement, affiliation, sponsorship, or recommendation: (i) by Mini-Circuits of such third-party's products, services, processes, or other information; or (ii) by any such third-party of Mini-Circuits or its products, services, processes, or other information.